

# Rapid SARS-CoV-2 Antigen Test


## User Instructions

A nasal swab sample can be self-collected by an individual aged 14 years and older. Children aged 2 to 13 years should be tested by an adult.




Scan QR code to navigate to digital instructions

## Kit Contents

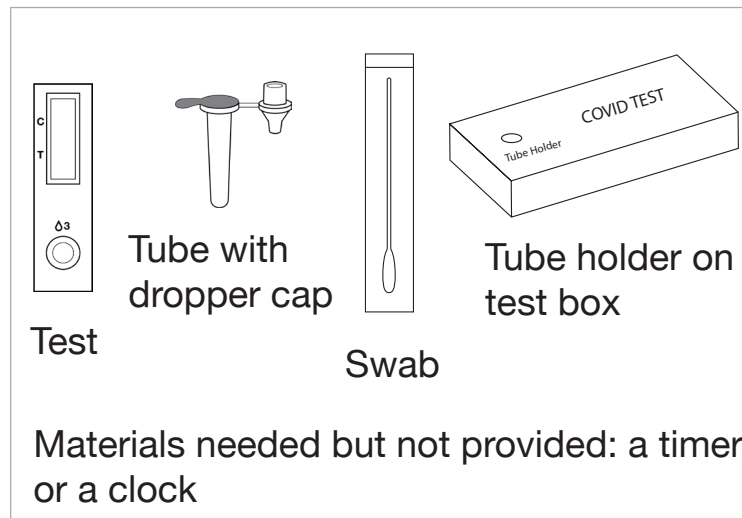






## Preparation

- 1 Wash your hands with soap and water, or use hand sanitizer, before performing the test.
- 2 Check test expiration date on the side of the test box.  
**WARNING: Do not proceed with an expired test.**




## Test Procedure


- 3 Push the tube into the perforated slot on the box labeled "Tube Holder"
- 4 Remove the seal from the tube.
- 5 Remove the test from the pouch and place it on a flat surface.
- 6 Peel open the swab packaging and remove the swab.  
**WARNING: Do not touch the soft tip of the swab**
- 7 Insert the swab 1/2 to 3/4 inches into the nostril. Gently rub the swab around the inside of the nostril while making 5 big circles. Do not just spin the swab.
- 8 Repeat Step 7 in the other nostril using the same swab.  
**WARNING: Inaccurate test results may occur if the nasal swab specimen is not properly collected. BOTH nostrils must be swabbed.**

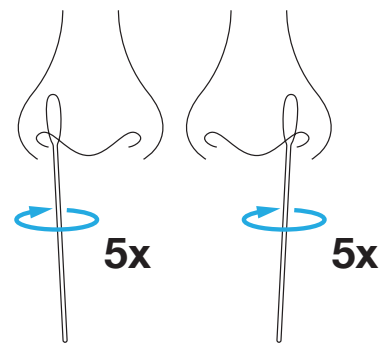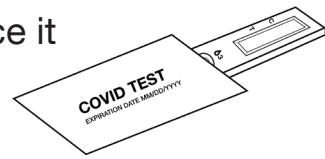


- 9 Place the swab in tube and rotate 5 times to mix.




- 10 Remove the swab from the tube and dispose of it in household trash.



- 11 Press the attached dropper cap on the tube until it clicks.




- 12 Invert the tube and squeeze 3 drops into the sample well on the test.

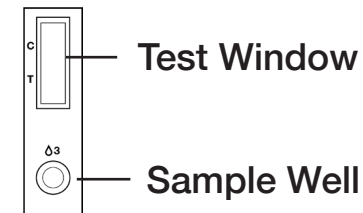

- 13 Set a timer for 15 minutes.

**WARNING: Do not read results before 15 minutes or after 30 minutes.**




15 minutes

## Results

Look at the result window and locate the letters C and T on the side of the window. A red line should always appear at the C position; this is a control line and signals that the test is working properly.

### Invalid Result




If the control (C) line is not visible, the test is invalid. Test again with a new swab and test device.

### Negative Result



If the Control (C) line is visible, but the Test (T) line is not visible, the test is negative. The virus that causes COVID-19 was not detected in your sample. You may still have COVID-19 and be contagious. If you test negative and continue to experience COVID-19-like symptoms, (e.g., fever, cough, and/or shortness of breath) you should seek follow up care with your health care provider.

### Positive Result



If the Control (C) line and the Test (T) line are visible, the test is positive. Any faint visible test (T) line with the control line (C) should be read as positive. A positive test result means that the virus that causes COVID-19 was detected in your sample and it is very likely you have COVID-19 and are contagious. Please contact your doctor/primary care physician or your local health authority immediately and adhere to the local guidelines regarding self-isolation.

## Disposal

All used components should be disposed of in household trash.